

Product testing MNS 03 according to DIN EN 14683

According to the investigations by Hohenstein Laboratories GmbH & Co. KG we confirm that you have passed the following tests:

- Bacterial filtration efficiency: $\geq 98\%$
- Differential pressure: $> 40 \text{ Pa/cm}^2$
- Microbial cleanliness: $\leq 30 \text{ KBE/g}$


The test for biocompatibility shows that no cytotoxic substances are released.

The tested probe does fulfil the requirements of DIN EN 14683 for medical masks type II.

Münster, 06/17/2020



Christopher Heine
CEO

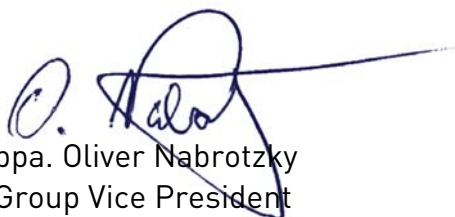

ppa. Oliver Nabrotzky
Group Vice President